

# Mouse IL-17A ELISA-KIT

Ref.: mIL-17A-EIA-5-KIT

MabTag's ELISA for mouse Interleukin-17A (mIL-17A) contains appropriate reagents sufficient for processing of 5 microplates (5 x 96 wells; 100 µl/well)

For research only. Not for use in diagnostic or therapeutic procedures.

**Specificity:** mouse Interleukin-17A (mIL-17A)

**Typical standard curve range:** 16 – 1000 pg/ml

**Detection limit:** 3.3 pg/ml

**Samples:** Culture supernatants, lysates, serum, plasma and other body fluids.


For serum and plasma a dilution of ≥ 1:10 is recommended.



**MabTag**  
GmbH

| Content   | Working dilution                               | Storage            |
|---|--|--------------------|
| 1 x vial 500 µl liquid anti-mIL-17A Capture-Antibody (red cap)      | 1:100  | -20°C              |
| 1 x vial 500 µl liquid anti-mIL-17A Detection-Antibody (yellow cap) | 1:100  | -20°C              |
| 1 x vial 50 ng lyophilized rmIL-17A Standard (white cap)            | customer specific                              | -20°C              |
| 1 x vial 50 µl Poly-HRP-Streptavidin (blue or green cap)            | 1:1000   | -20°C              |
| 5 x 96well-Microplate   | -  | room temperature   |
| 1 x 60 ml Coating-Buffer  | ready-to-use                                   | 2-8°C              |
| 3 x 100 ml Blocking-Buffer / Reagent-Diluent                        | ready-to-use                                   | 2-8°C              |
| 3 x 100 ml Wash-Buffer (10x concentrated)                           | 100 ml must be filled up to 1L with aqua dest. | 2-8°C              |
| 1 x 4 ml TMB-Solution A   | 10 ml TMB-B + 0.5 ml TMB-A                     | 2-8°C              |
| 1 x 60 ml TMB-Solution B  |  | protect from light |
| 1 x 30 ml Stop-solution ACID → wear gloves & protective glass       | ready-to-use                                   | 2-8°C              |

## Typical standard curve

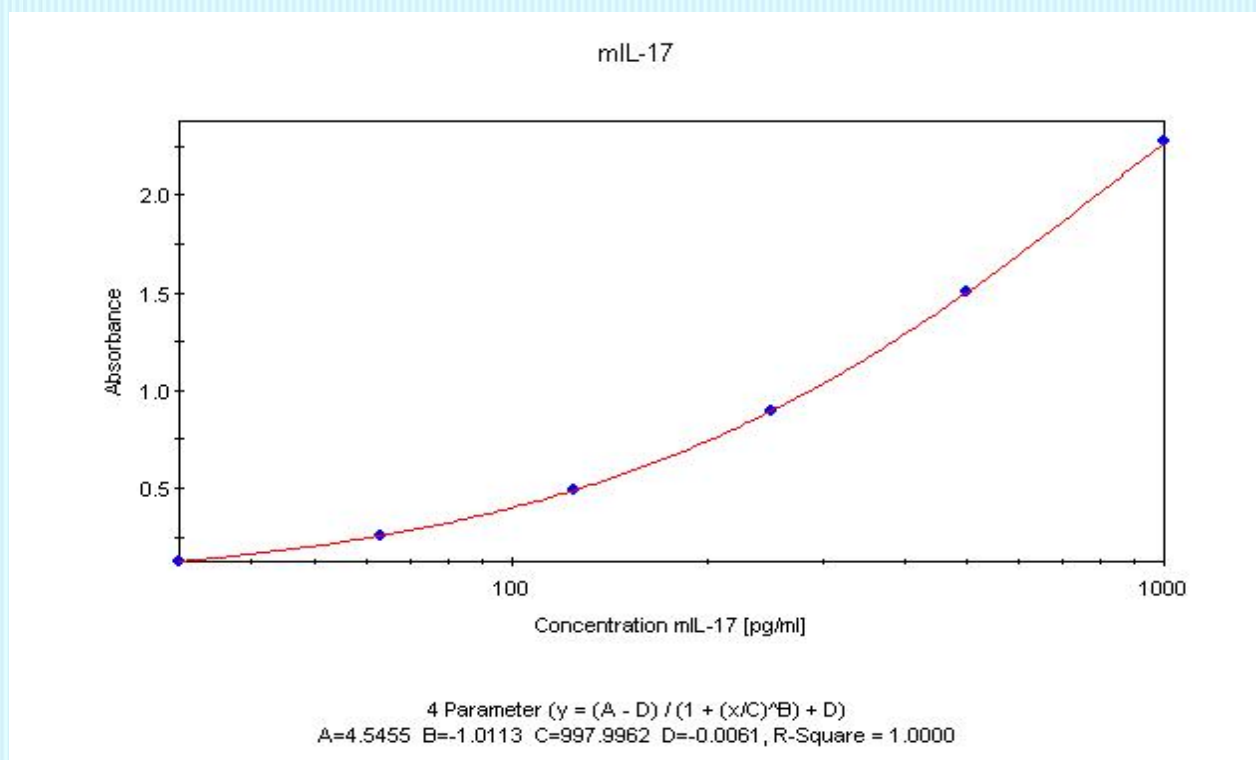

**!Spin down all vials before use!**

| Step   | Incubation  | Procedure   |
|--|---|---|
| <b>Coating<br/>Capture-antibody</b>  | ≥ OVERNIGHT<br>at room<br>temperature                         | Dilute <b>capture-antibody</b> 1:100 in COATING-BUFFER<br>(100 µl capture-antibody in 10 ml COATING-BUFFER).<br>Subsequently transfer 100 µl of this working-solution to each well and incubate.  |
| Remove capture-antibody completely by inverting the microplate and blotting it <b>vigorously</b> against clean paper towels.   |   |   |
| <b>Blocking</b>  | ≥ 1 Hour<br>at room<br>temperature                            | Add 300 µl BLOCKING-BUFFER to each well and incubate.   |
| Remove BLOCKING-BUFFER completely by inverting the microplate and blotting it <b>vigorously</b> against clean paper towels.  |   |   |
| <b>Standard &amp;<br/>Sample</b>   | ≥ 2 Hours<br>at room<br>temperature                           | Dilute <b>standard</b> & samples in REAGENT-DILUENT and transfer 100 µl in the respective wells in duplicates. Standard: Make serial dilutions in REAGENT-DILUENT and begin with a high standard and end with blanks. The standard vial of this set contains <b>50 ng lyophilized standard</b> . Reconstitute this in exactly 1 ml REAGENT-DILUENT (stock solution = 50 ng/ml) and choose a sufficient high standard working solution for your assay (e.g. prepare a 1:20 dilution for a standard curve beginning with 2500 pg/ml). |
| Wash 5x <b>vigorously</b> with WASHING-BUFFER and remove resting buffer completely by inverting the microplate and blotting it <b>vigorously</b> against clean paper towels. |   |   |
| <b>Detection-<br/>antibody</b>   | ≥ 2 Hours<br>at room<br>temperature                           | Dilute <b>detection-antibody</b> 1:100 in REAGENT-DILUENT<br>(100 µl detection-antibody in 10 ml REAGENT-DILUENT).<br>Subsequently transfer 100 µl of this working-solution to each well and incubate.  |
| Wash 5x <b>vigorously</b> with WASHING-BUFFER and remove resting buffer completely by inverting the microplate and blotting it <b>vigorously</b> against clean paper towels. |   |   |
| <b>Poly-HRP-<br/>Streptavidin</b>  | <b>20-30 Min</b><br>at room<br>temperature                    | Dilute <b>Poly-HRP-Streptavidin</b> 1:1000 in REAGENT-DILUENT<br>(10 µl in 10 ml REAGENT-DILUENT).<br>Subsequently transfer 100 µl of this working-solution to each well and incubate.  |
| Wash 5x <b>vigorously</b> with WASHING-BUFFER and remove resting buffer completely by inverting the microplate and blotting it <b>vigorously</b> against clean paper towels. |   |   |
| <b>Substrate<br/>solution</b>  | Up to 60 Min*<br>at room<br>temperature<br><b>in the dark</b> | Optionally warm the solution to room temperature before use.<br>Add 100 µl of the SUBSTRATE-SOLUTION to each well and incubate.<br>Control the development of the colour reaction continuously and stop at an appropriate time point.   |
| <b>Stop solution</b>   | -   | When the enzymatic colour reaction is sufficiently proceeded stop the reaction by adding of 50 µl stop solution. Read the microplate at the substrate-depending wavelength. (e.g. <b>450 nm</b> for TMB substrate)<br>(if wavelength correction is available, set to 540 nm, 570 nm or 630 nm as reference)   |

\*The speed of enzymatic colour development is influenced by many customer-specific factors. Therefore the incubation time is variable und specific for each test system.

**Note:**

All incubation steps except TMB substrate could be optionally carried out over-night. Do not use sodium azide-containing solutions, nor add sodium azide to the supplied reagents. Sodium azide inactivates the peroxidase.

**Storage:**

Specific storage conditions in the table above.

Reconstituted reagents should be stored at -20°C. Please prevent repeated freeze- thaw cycles. Stable for up to 6 months after opening when stored at -20° C. The performance of the unopened reagents is guaranteed until one year after point of delivery.

**Precautions for use:**

!The stop solution is an acid solution. TMB-Solution A contain  $H_2O_2$  and tetramethylbenzidine (TMB). All Buffers and liquid antibody solutions contain 0.045% (v/v) Proclin®950 as preservative. All these compounds are harmful and cause respiratory, skin and eye irritation. Do not swallow any components of the set/kit (R22). Wear face, eye and hand clothing protection when using this material (S36). Keep out of reach of children (S2). Keep away from food, drink and animal feeding stuff (S13). !These reagents are offered for research purposes only! For *in vitro* use only. MabTag will not be held responsible for patent infringement or other violations that may occur with the use of our products.

ProClin is a registered trade mark of Rohm and Haas Company.